
BLS Healthcare Provider Adult Cardiac Arrest Algorithm-2015 Update

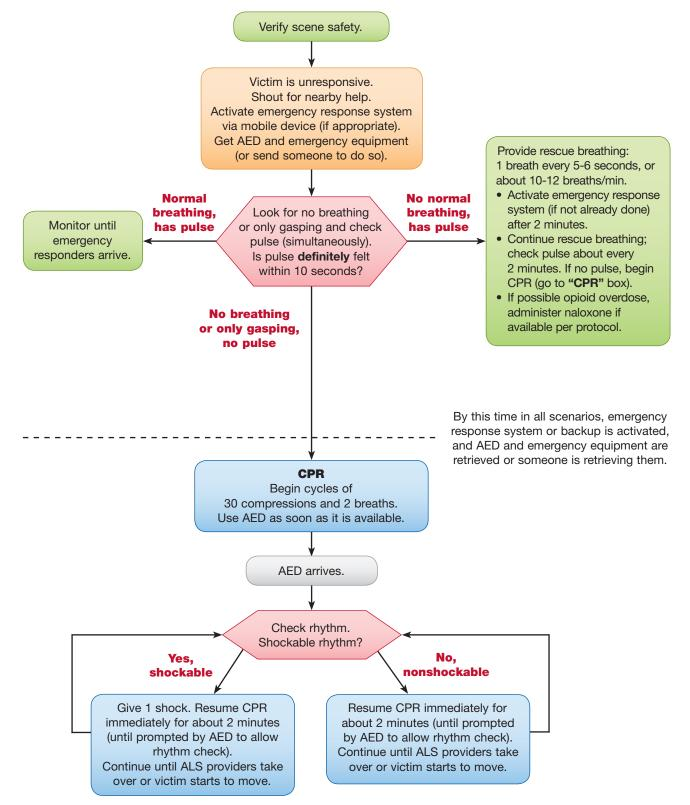

Summary of High-Quality CPR Components for BLS Providers

Component	Adults and Adolescents	Children (Age 1 Year to Puberty)	Infants (Age Less Than 1 Year, Excluding Newborns)
Scene safety	Make sure the environment is safe for rescuers and victim		
Recognition of cardiac arrest	Check for responsiveness No breathing or only gasping (ie, no normal breathing) No definite pulse felt within 10 seconds (Breathing and pulse check can be performed simultaneously in less than 10 seconds)		
Activation of emergency response system	If you are alone with no mobile phone, leave the victim to activate the emergency response system and get the AED before beginning CPR Otherwise, send someone and begin CPR immediately; use the AED as soon as it is available	Witnessed collapse Follow steps for adults and adolescents on the left Unwitnessed collapse Give 2 minutes of CPR Leave the victim to activate the emergency response system and get the AED Return to the child or infant and resume CPR; use the AED as soon as it is available	
Compression-ventilation ratio without advanced airway	1 or 2 rescuers 30:2	<i>1 rescuer</i> 30:2 <i>2 or more rescuers</i> 15:2	
Compression-ventilation ratio with advanced airway	Continuous compressions at a rate of 100-120/min Give 1 breath every 6 seconds (10 breaths/min)		
Compression rate	100-120/min		
Compression depth	At least 2 inches (5 cm)*	At least one third AP diameter of chest About 2 inches (5 cm)	At least one third AP diameter of chest About 1½ inches (4 cm)
Hand placement	2 hands on the lower half of the breastbone (sternum)	2 hands or 1 hand (optional for very small child) on the lower half of the breastbone (sternum)	 <i>1 rescuer</i> 2 fingers in the center of the chest, just below the nipple line <i>2 or more rescuers</i> 2 thumb–encircling hands in the center of the chest, just below the nipple line
Chest recoil	Allow full recoil of chest after each compression; do not lean on the chest after each compression		
Minimizing interruptions	Limit interruptions in chest compressions to less than 10 seconds		

*Compression depth should be no more than 2.4 inches (6 cm).

Abbreviations: AED, automated external defibrillator; AP, anteroposterior; CPR, cardiopulmonary resuscitation.

Positions for 6-Person High-Performance Teams*

Resuscitation Triangle Roles

Compressor

- Assesses the patient
- Does 5 cycles of chest compressions
- Alternates with AED/Monitor/ Defibrillator every 5 cycles or 2 minutes (or earlier if signs of fatigue set in)


AED/Monitor/ Defibrillator

- Brings and operates the AED/monitor/defibrillator
- Alternates with Compressor every 5 cycles or 2 minutes (or earlier if signs of fatigue set in), ideally during rhythm analysis
- If a monitor is present, places it in a position where it can be seen by the Team Leader (and most of the team)

Airway

- Opens and maintains the airway
- Provides ventilation


The team owns the code. No team member leaves the triangle except to protect his or her safety.

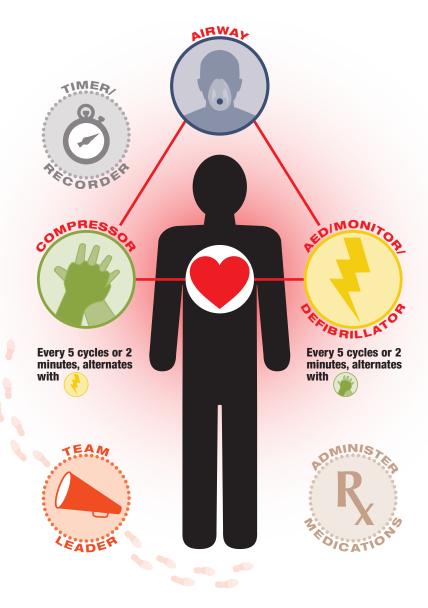



Leadership Roles Team Leader Every resuscitation team must have a defined leader · Assigns roles to team members Makes treatment decisions • Provides feedback to the rest of the team as needed • Assumes responsibility for roles not assigned Administer **Medications** • An ALS provider role Administers medications Timer/Recorder · Records the time of interventions and medications (and announces when these are next due) • Records the frequency and duration of interruptions in compressions • Communicates these to the Team Leader (and the rest of the team)

Adult Cardiac Arrest Circular Algorithm – 2018 Update

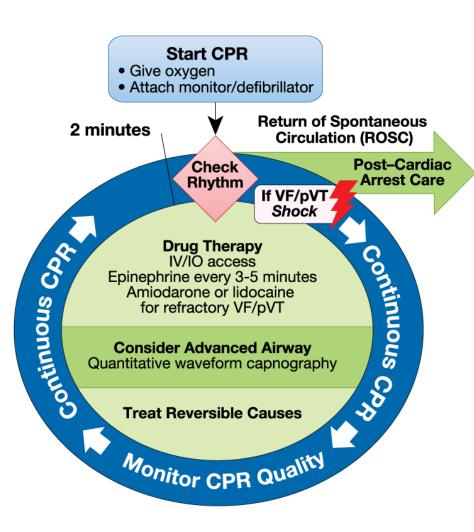

CPR Quality

- Push hard (at least 2 inches [5 cm]) and fast (100-120/min) and allow complete chest recoil.
- Minimize interruptions in compressions.
- Avoid excessive ventilation.
- Change compressor every 2 minutes, or sooner if fatigued.
- If no advanced airway, 30:2 compression-ventilation ratio.
- Quantitative waveform capnography
 - If PETCO₂ <10 mm Hg, attempt to improve CPR quality.
- Intra-arterial pressure
- If relaxation phase (diastolic) pressure <20 mm Hg, attempt to improve CPR quality.

Shock Energy for Defibrillation

- **Biphasic:** Manufacturer recommendation (eg, initial dose of 120-200 J); if unknown, use maximum available. Second and subsequent doses should be equivalent, and higher doses may be considered.
- Monophasic: 360 J

Drug Therapy

- Epinephrine IV/IO dose: 1 mg every 3-5 minutes
- Amiodarone IV/IO dose: First dose: 300 mg bolus. Second dose: 150 mg.
 -OR-

Lidocaine IV/IO dose: First dose: 1-1.5 mg/kg. Second dose: 0.5-0.75 mg/kg.

Advanced Airway

- · Endotracheal intubation or supraglottic advanced airway
- Waveform capnography or capnometry to confirm and monitor ET tube placement
- Once advanced airway in place, give 1 breath every 6 seconds
 (10 breaths/min) with continuous chest compressions

Return of Spontaneous Circulation (ROSC)


- Pulse and blood pressure
- Abrupt sustained increase in PETCO₂ (typically ≥40 mm Hg)
- · Spontaneous arterial pressure waves with intra-arterial monitoring

Reversible Causes

- Hypovolemia
- Hypoxia
- Hydrogen ion (acidosis)
- Hypo-/hyperkalemia
- Hypothermia


- Tension pneumothorax
- Tamponade, cardiac
- Toxins
- Thrombosis, pulmonary
- Thrombosis, coronary

Adult Cardiac Arrest Algorithm – 2018 Update

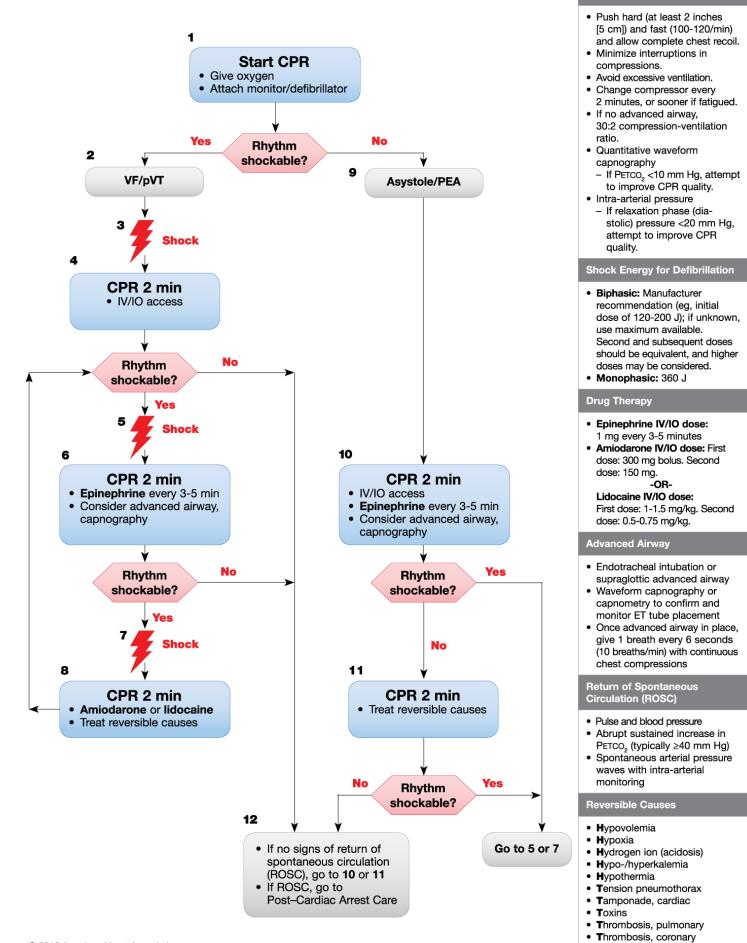


CPR Quality

Adult Immediate Post-Cardiac Arrest Care Algorithm - 2015 Update

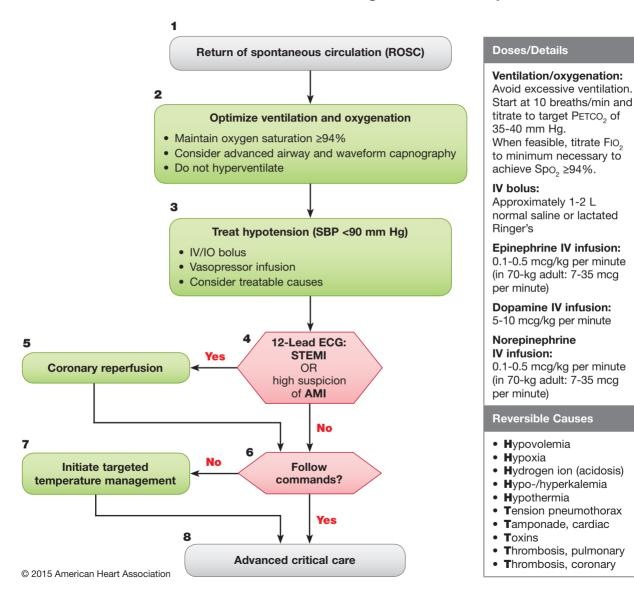

Adult Bradycardia With a Pulse Algorithm

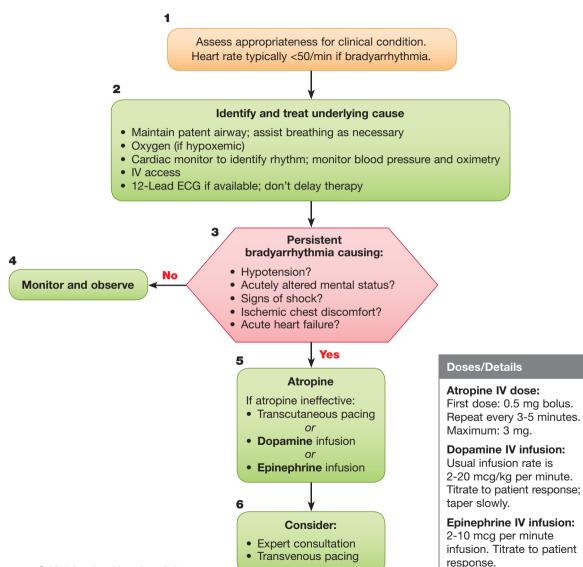

© 2015 American Heart Association

Adult Tachycardia With a Pulse Algorithm

